


**Quality in Water Analysis**  
**██████████ - Institute for Oceanography and**  
**fisheries**  
**Individual Report**  
**Round: 169**

Issue Number 1

Issued 28 May 2010

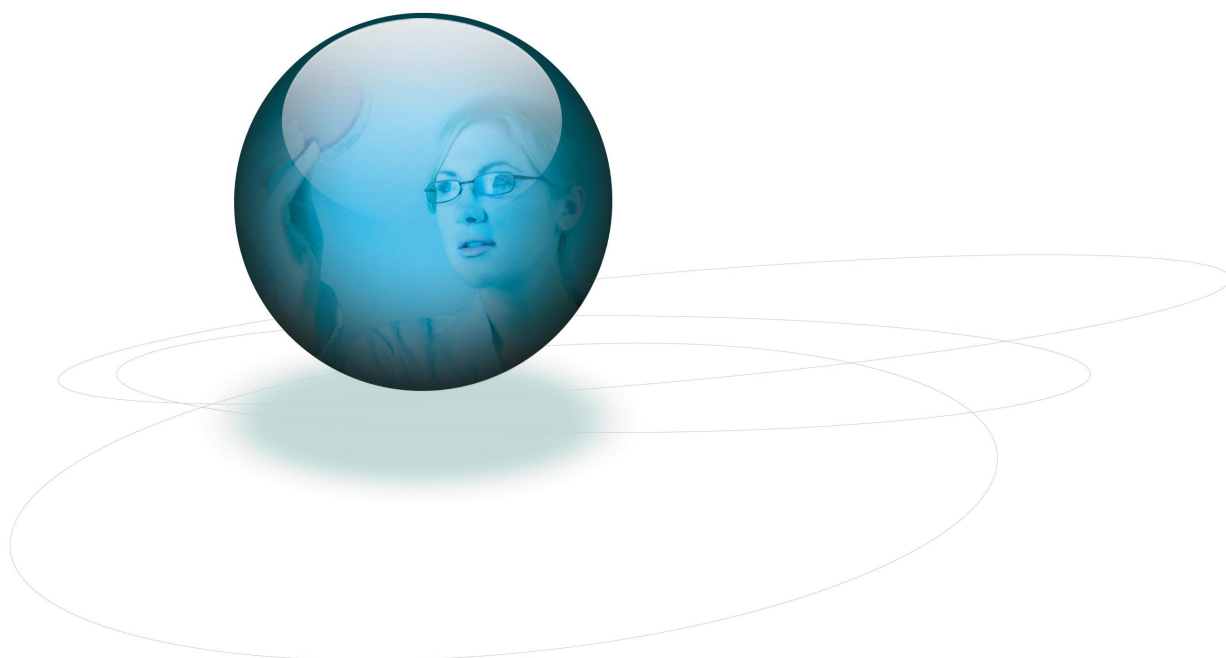

## Individual Report

This individual report contains a summary of all the results submitted and the performance assessments for your laboratory and your individual analysts. Please note that nominated laboratory results are represented by a blue highlight in the analyst box.

Data statistics given in the individual report are for the method you have used for each analyte. Further detail can be obtained from the main report.

Full details of the scheme, sample types, analytes and data analysis can be found in the corresponding Main Report, along with any technical comments, if applicable. The Main Report is the definitive version.

If you have any questions regarding your results which are not answered in the Main Report, please contact us using the details on the front of the report. If you would like to order any samples for re-test, please contact our customer service department or your local office.

## Results Summary

Sample	Results Reported	Satisfactory Results	Questionable Results	Unsatisfactory Results	Not Assessed
419 - Surface/Waste/Bathing Water	20	20	0	0	0
<b>Round Total</b>	<b>20</b>	<b>20</b>	<b>0</b>	<b>0</b>	<b>0</b>

No unsatisfactory results in this round

No questionable results in this round

## 419 - Surface/Waste/Bathing Water

Analyte	Analyst	Method	Result	Units	z score	Assigned Value	Uncertainty	SDPA	No of results	Median	Mean	Robust SD	SD
Total coliforms	MO	Other	3,500	cfu/100ml	-0.07	3,700	0.02	0.35	51	3.59	3.52	0.13	0.27
Total coliforms	DS	Other	2,250	cfu/100ml	-0.62	3,700	0.02	0.35	51	3.59	3.52	0.13	0.27
Total coliforms	SJ	Other	3,630	cfu/100ml	-0.02	3,700	0.02	0.35	51	3.59	3.52	0.13	0.27
Total coliforms	SS	Other	3,030	cfu/100ml	-0.25	3,700	0.02	0.35	51	3.59	3.52	0.13	0.27
Faecal coliforms	SJ	Other	3,480	cfu/100ml	0.38	2,572	0.03	0.35	61	3.40	3.34	0.25	0.33
Faecal coliforms	DS	Other	3,540	cfu/100ml	0.40	2,572	0.03	0.35	61	3.40	3.34	0.25	0.33
Faecal coliforms	MO	Other	3,000	cfu/100ml	0.19	2,572	0.03	0.35	61	3.40	3.34	0.25	0.33
Faecal coliforms	SS	Other	3,280	cfu/100ml	0.30	2,572	0.03	0.35	61	3.40	3.34	0.25	0.33
Escherichia coli	MO	Other	3,570	cfu/100ml	0.22	3,000	0.03	0.35	44	3.32	3.25	0.34	0.39
Escherichia coli	DS	Other	3,900	cfu/100ml	0.33	3,000	0.03	0.35	44	3.32	3.25	0.34	0.39
Escherichia coli	DS	MEMF Chromogeni c agar 37	4,060	cfu/100ml	0.38	3,000	0.03	0.35	16	3.49	3.31	0.22	0.44
Escherichia coli	MO	MEMF Chromogeni c agar 37	4,217	cfu/100ml	0.42	3,000	0.03	0.35	16	3.49	3.31	0.22	0.44
Escherichia coli	SJ	Other	3,580	cfu/100ml	0.22	3,000	0.03	0.35	44	3.32	3.25	0.34	0.39
Escherichia coli	SJ	MEMF Chromogeni c agar 37	4,217	cfu/100ml	0.42	3,000	0.03	0.35	16	3.49	3.31	0.22	0.44
Escherichia coli	SS	Other	3,460	cfu/100ml	0.18	3,000	0.03	0.35	44	3.32	3.25	0.34	0.39
Escherichia coli	SS	MEMF Chromogeni c agar 37	4,350	cfu/100ml	0.46	3,000	0.03	0.35	16	3.49	3.31	0.22	0.44
Enterococci (faecal streptococci)	SJ	MEMF SB 37	463	cfu/100ml	-0.08	495	0.02	0.35	85	2.71	2.68	0.12	0.13
Enterococci (faecal streptococci)	DS	MEMF SB 37	453	cfu/100ml	-0.11	495	0.02	0.35	85	2.71	2.68	0.12	0.13
Enterococci (faecal streptococci)	MO	MEMF SB 37	490	cfu/100ml	-0.01	495	0.02	0.35	85	2.71	2.68	0.12	0.13
Enterococci (faecal streptococci)	SS	MEMF SB 37	536	cfu/100ml	0.10	495	0.02	0.35	85	2.71	2.68	0.12	0.13